



CIT CR TEST PHANTOM FOR RADIOGRAPHIC SYSTEM QUALIFICATION

INTRODUCTION

The need for Quality Control is emphasised throughout any production system. Measurement and traceability of equipment performance, and assurance of repeatability and accuracy, are paramount in establishing correct working practices. Checking the performance of a Radiographic System for Quality Assurance purposes has historically been an arduous task, with differing standards and multiple test gauges and exposures.

CIT's CR Test Phantom incorporates the required test elements into a **Single simple-to-use unit**, allowing the evaluation of Computed Radiography (CR) systems for industrial radiography in accordance with ASTM and EN International Radiographic Testing standards as well as monitoring the quality of the chosen system

The regular use of the CR Test Phantom will assure the **long-term stability**-performance measurements of the CR system over the life-cycle of the devices

BASIC RADIOGRAPHIC MEASUREMENT PERFORMANCE

There are several factors affecting the quality of a CR image, including the spatial resolution of the IP system, geometrical unsharpness, scatter and contrast sensitivity (signal/noise ratio). There are several additional factors (for example scanning parameters) that affect the accurate reading of displayed digital images

The CR Phantom provides the quality indicators for measuring of:

- Shading
- Spatial resolution
- Central beam alignment
- Converging Gauge - 20Lp/M
- Radiograph Set-Up Unsharpness
- MTF
- Jitter
- Linearity
- Slipping
- Contrast Sensitivity

SIZE

CIT CR Phantom comes in two sizes. 8" x 10" and 14" x 17"




STANDARD REFERENCES

The CIT Test Phantom is designed to fully comply with the requirements of

- ASTM E2445-05 Appendix X1, • EN 14784-1:2005.
- ASTM E2002 / EN462-5 • ASTM 1647-98a

ORDERING INFORMATION

Item	8" x 10"(203 x 254mm)	14" x 17"(356 x 432mm)
Phantom	CIT/CR-Phan 0810	CIT/CR-Phan 1417

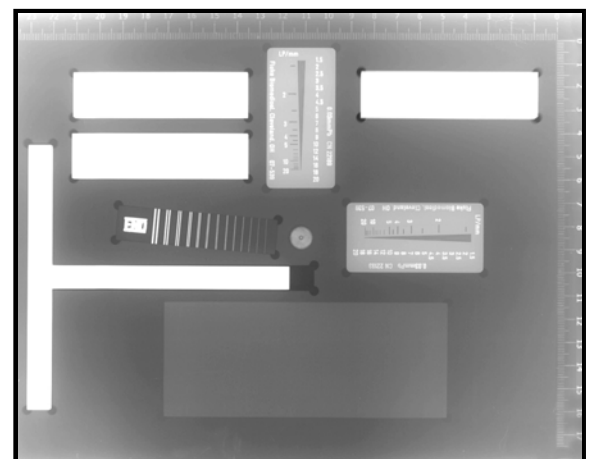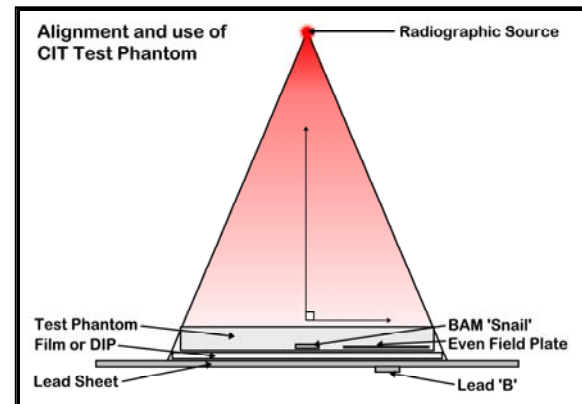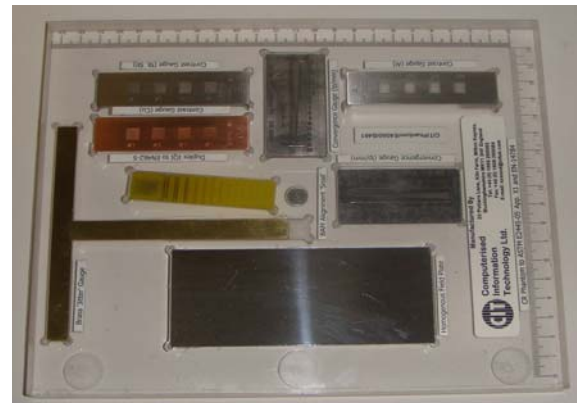

For further details please contact CIT at the below address



**Manufacturer of the World's Most Advanced Imaging,
Digital Radiography and Archive Systems**